




# Usage data collection made easier with MyLink™

## About MyLink


MyLink enables you to easily upload your Optune® device data to the remote storage server from the comfort of your home.

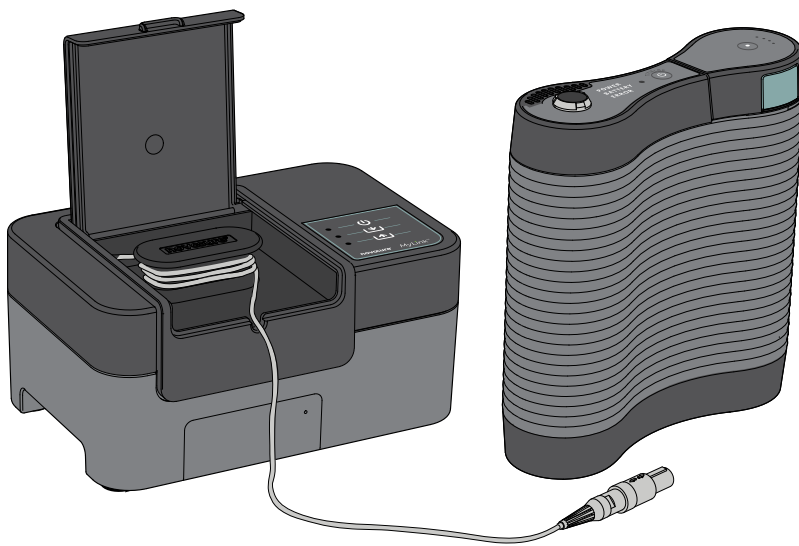


## MyLink and its indicators next to the Optune device



MyLink

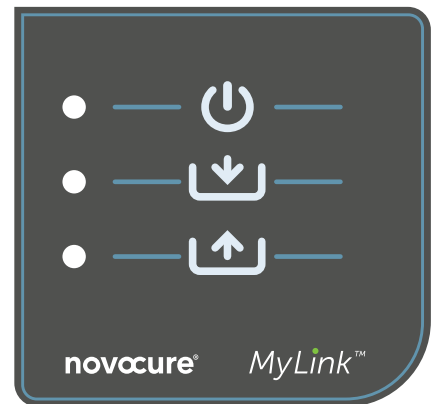Optune device



-  On/off indicator
-  Downloading treatment data indicator
-  Uploading treatment data indicator

**WARNING!**—All servicing procedures must be performed by qualified and trained personnel. Attempting to open and service the system may result in an electric shock by touching the inner parts of the equipment. It could also cause damage to the system.

**WARNING!**—No modification of this equipment is allowed.

Note: the unit is using a cellular network for its operation. If you are trying to use it in a non-cellular reception environment, the unit will not work properly.

MyLink is to be used with Optune model TFH9100 only.

For questions about MyLink™ or services available to you, contact nCompass™ via phone or email.




Call us toll free:  
**1-855-281-9301 (toll free)**




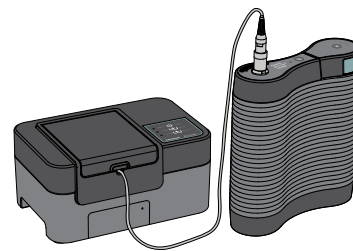
Or email us:  
[support@novocure.com](mailto:support@novocure.com)

# Using your MyLink™



MyLink


1. Plug the cord into the back side of the MyLink unit and then connect the unit to a wall outlet. Press the switch to "I" to power on the unit. Wait until the  indicator stops blinking and turns steady green.




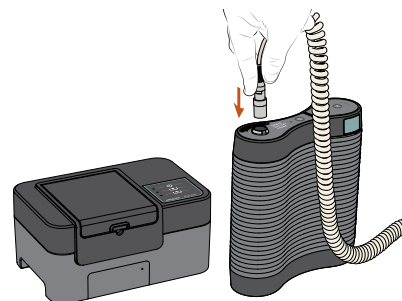
MyLink

Optune device

2. Stop TTFields therapy by pressing the TTFields button on your Optune device, and unplug the connection cable from your Optune device. Connect the MyLink cable located under the lid of your MyLink unit to your Optune device. To ensure proper connection, line up the arrows on the MyLink cord to the arrow on the Optune device.





3. Make sure that your Optune device is turned on. The  indicator on the top of your MyLink unit blinks green as MyLink downloads your data.





MyLink

Optune device

4. When the  indicator stops blinking and turns steady green and the MyLink beeps, the data has been downloaded. You can now disconnect the MyLink cable. Your Optune device will perform a quick reset. Once the reset is completed, you can resume your treatment.



5. When the  light blinks green, your MyLink unit is uploading your treatment data directly to the server. This takes up to 15 minutes.



MyLink

6. When all 3 lights stop blinking and turn steady green, the upload is successful. You can now turn off your MyLink unit and unplug it from the wall outlet.